

**NETZSCH**

Proven Excellence.



Dilatometer Series

DIL 402 *Expedis*® *Select, Supreme and Supreme HT*

Method, Instruments, Applications

Analyzing & Testing

# Dilatometry



# The Method for Determination of Dimensional Changes

Each time a material is exposed to temperature changes – it shows a variation in its dimension. Whether it is in the course of its regular thermal expansion, by passing a phase transition or while it undergoes sintering, the substance will either be shrunk or elongated.


Dilatometry is the method of choice to study length change phenomena of ceramics, glasses, metals, composites, and polymers as well as other construction materials, thus revealing information regarding their thermal behavior and about process parameters or sintering (and curing) kinetics.

For preparing a dilatometer measurement, the defined sample is inserted into a sample holder and brought into contact with the pushrod. After closing the furnace, the experiment can be started.

Thermal expansion of the sample during heating is detected by the displacement system which the pushrod is connected to.

## Results obtainable by DIL measurements

- Linear thermal expansion
- Coefficient of thermal expansion (CTE)
- Volumetric expansion
- Shrinkage steps
- Softening point
- Glass transition temperature
- Phase transitions
- Sintering temperature and step
- Density change
- Influence of additives and raw materials
- Decomposition temperature of e.g., organic binders
- Anisotropic behavior
- Optimizing of firing process
- Caloric effects by using *c-DTA*®
- Rate-Controlled Sintering (RCS)
- Kinetics Neo

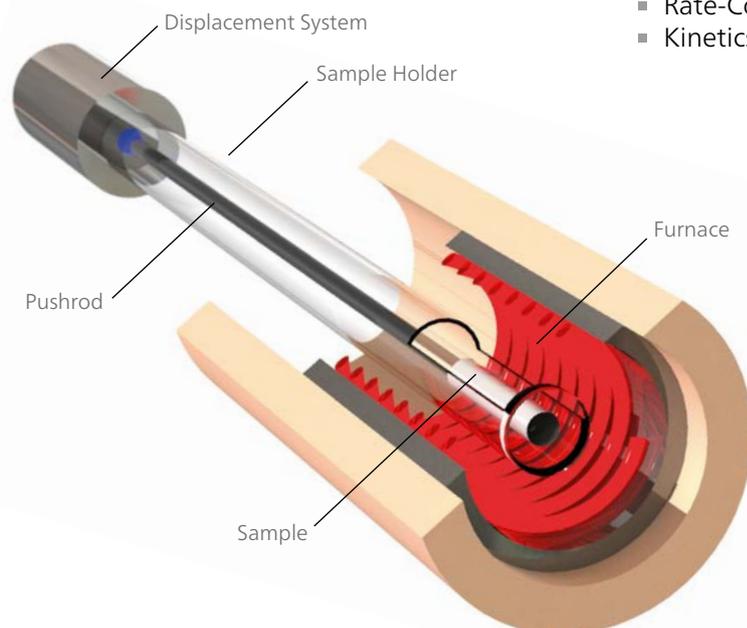

# Dilatometry Redefined

## MAXIMUM FLEXIBILITY

The double furnace sliding carrier of the DIL 402 *Expedis*<sup>®</sup> *Select/Supreme* standard versions creates the opportunity to cover the entire temperature range from -180°C to 2000°C or, alternatively, to increase the sample throughput by having two furnaces available for use.

## UTMOST VERSATILITY

Due to the wide dynamic range of the measurement system, it is possible to measure both soft and hard samples without impairment of the properties. Additionally, it enables force modulation and builds a bridge to thermo-mechanical analysis (TMA).



## NanoEye – LARGEST MEASURING RANGE, HIGHEST RESOLUTION

The new, pioneering opto-electronic NanoEye displacement system features perfect linearity and maximum resolution over a measuring range which was impossible to realize until now.

Instrument Type	Resolution	Measuring Range
Select	1 nm	± 10 mm
Supreme	0.1 nm	± 25 mm

## USER-OPTIMIZED DESIGN

A wide force range for more fragile samples, built-in mass flow controllers and electrical thermostating of the measuring cell to suppress any temperature influence from the surrounding provide for ease-of-use and maximum operational safety.

ALL-IN-ONE DESIGN  
 MODULAR CONCEPT  
 SINGLE OR DOUBLE DILATOMETER  
 HIGH SAMPLE THROUGHPUT  
 LOW COST OF OPERATION  
 FAST START OF MEASUREMENT  
 WIDE TEMPERATURE RANGE  
 TUBE TYPE SAMPLE HOLDERS  
 ROD TYPE SAMPLE HOLDERS  
 FORCE MODULATION  
 FURNACE VARIETY  
 MOTORIZED FURNACE  
 EXCHANGEABLE FURNACES  
 ROBUST  
**NANO EYE**  
 HIGHEST RESOLUTION  
 PERFECT LINEARITY  
 CONSTANT RESOLUTION  
**USER-OPTIMIZED DESIGN**  
 EASE OF USE  
 INNOVATIVE FORCE CONTROL  
 HIGHEST PRECISION  
**FLEXIBILITY**  
 VARIABLE CONTACT FORCE  
 FRAGILE SAMPLES  
 HIGHEST REPRODUCIBILITY  
**UTMOST VERSATILITY**  
 AUTOMATIC LENGTH  
 DETERMINATION  
 SOFT SAMPLES  
 CUSHIONING OF THE FURNACE  
 ISOLATED MEASUREMENT CELL  
 NO CHILLER  
 PRECISE CONTACT FORCE  
 CONSTANT CONTACT FORCE  
 LARGE MEASUREMENT RANGE  
 SLIDING THERMOCOUPLE  
 LONG-TERM MEASUREMENTS  
 DEMANDING APPLICATIONS  
 GAS-TIGHT ENVIRONMENT  
 DEFINED ATMOSPHERE  
 MASS FLOW CONTROLLER  
 SIMPLIFIED SAMPLE HOLDER CHANGE  
 FAST & EASY FURNACE CHANGE  
 SOLID SAMPLE HOLDERS  
 EASY CLEANING




# NanoEye

## A New Dimension in Measuring Range and Accuracy

In classical dilatometry, the two parameters **measurement range** and **resolution** mostly seem diametrically opposed. If the resolution goes up, the measuring range usually goes down and vice versa.

*NanoEye*, the novel opto-electronic displacement system, is able to overcome this conflict and offers **highest resolution** associated with an **unmatched measuring range**.

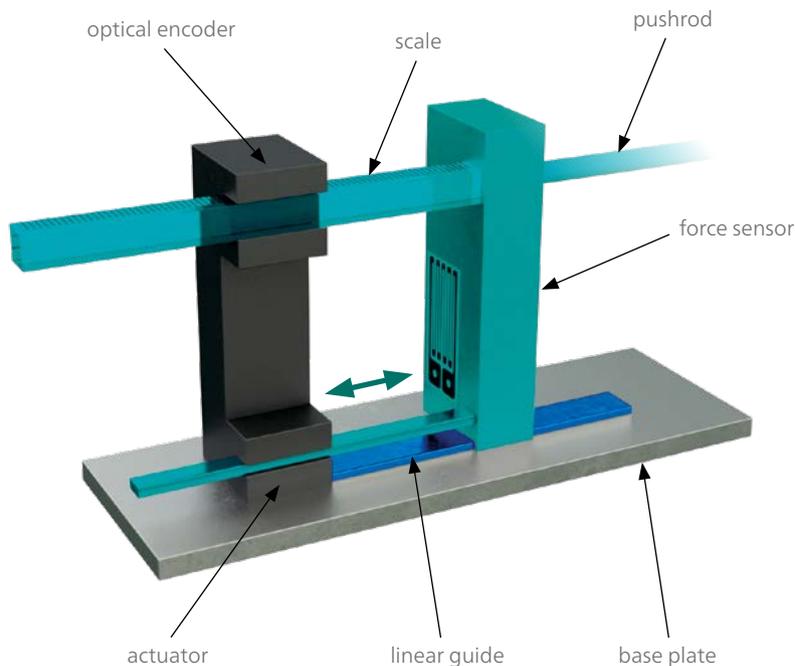

Schematic of the *NanoEye* measuring cell

### Functional Principle

During a test run, if the sample expands, all **green** components in the graphics move backwards with the help of a linear guide (marked in **blue**). The optical encoder determines the corresponding length change directly on the appropriate scale.

### The *NanoEye* consists of:

- an actuator which applies a controlled contact force and moves the pushrod for adjusting variable sample lengths
- an elastic force sensor which detects the contact force subsequently enabling a force control cycle
- an optical encoder (plus scale) which measures the initial sample length and determines the length change of the sample



## Advantages using *NanoEye*

### Perfect Linearity

compared to conventional transducer systems – for measurements with large thermal expansion and unmatched linearity.

### Wider Measuring Range Than Ever Before

up to a factor of 10 compared to traditional dilatometers – for measurements on a large variety of different sample lengths with different thermal expansion behavior without manual adaption of measuring range.

### Friction-Free Construction

without sliding or rolling friction and stick-slip effects – for highest reproducibility of results.

### Displacement Determination with Nanometer Resolution

over the entire measuring range – for detecting even the smallest effects at every temperature.

### Controlled Contact Force During the Entire Measurement

for measurements on small, delicate, fragile or foamed samples without risk of non-reproducible deformation.

### Extremely Small Forces

adjustable for measurements on green bodies or soft samples.

### Maintenance-Free

The two standard versions of the DIL 402 *Expedis*<sup>®</sup> are specially designed for both research & development and sophisticated industrial applications: The comprehensive, fully-equipped *Supreme* model and the upgradable *Select* type (for a detailed comparison between the two models see page 25).

## Designed to Master the Challenges of the Future

### Optimum Adaptability

One or two furnaces, manual or motorized furnace operation, single or dual sample holders, tube type or rod type sample holders ... these are only some of the features the *Expedis*<sup>®</sup> *Select* or *Supreme* provide to match nearly all application scenarios.

### High Sample Throughput

The combination between the double furnace design and a dual sample holder used in dual mode increases the number of possible measurements tremendously and boosts the instrument's efficiency.





## Greatest Variability in Contact Force

The DIL 402 *Expedis*<sup>®</sup> series is the first horizontal dilatometer series on the market which allows for force modulation and, by this means, bridges the gap between dilatometry and thermomechanical analysis under oscillatory load.

For test runs under static force conditions, different contact forces can be selected. Therefore, both models are ideally suited to measure not only soft samples but also rigid, fragile materials.

## Widest Temperature Range from -180°C to 2000°C

To cover this temperature range, different furnaces are available and can be used both in the single furnace and double furnace format.

Furnace Type/Heating Element	Max. Temperature Range
Copper	-180°C ... 500°C
Stainless Steel	-150°C ... 1000°C
Fused Silica (SiO <sub>2</sub> )	RT ... 1150°C
Silicon Carbide (SiC)	RT ... 1600°C
Graphite	RT ... 2000°C

*Best Features of DIL 402  
Expedis<sup>®</sup> Select/Supreme –  
Standard Versions*

# Smart Usability Means More Than Just “Easy to Use”

## Automatic Sample Length Detection

Measuring the sample length with a caliper runs the risk of result scatter, especially for soft samples. The DIL 402 *Expedis*® is capable of detecting the initial length of a sample automatically prior to the start of a test run under conditions identical to those during the measurement itself.

## Large Measurement Range with Constant Resolution

In the past, it was often necessary to adapt the measuring range to the expected expansion or shrinkage of the sample to avoid signal overflow. With the new DIL 402 *Expedis*®, this is no longer the case. There is just one measuring range which is wide enough to quantify even the largest dimensional changes with a constant high resolution .

## Perfect Temperature Stability of the Measuring System

Thanks to the elaborate electrical temperature control of the *NanoEye*, the measurement signal is not affected by environmental temperature fluctuations.

## Temperature Measurement at the Right Spot

In order to conveniently measure various sample lengths, the thermocouple (if used) is adjustable. A guiding rod accommodates the thermocouple to place it in the desired position without bending.




## *MultiTouch*

A stable position of the sample inside the sample holder is a deciding factor for successful measurement results. The *MultiTouch* feature places the sample into the optimum position using a unique, tail-like motion.


# Outstanding Conditions for Pure Atmospheres

## Separate Gas Paths for Protective and Purge Gases

When using the three mass flow controllers (MFC, optional), the gas flow paths inside the instrument are split: the protective gas first passes through the measuring cell and then enters the sample chamber, whereas the purge gas(es) are directly fed into the sample chamber. All protective and purge gases leave the instrument together via the furnace exhaust. In the standard version, if only one MFC is integrated, the gas takes the same path as the protective gas mentioned above.

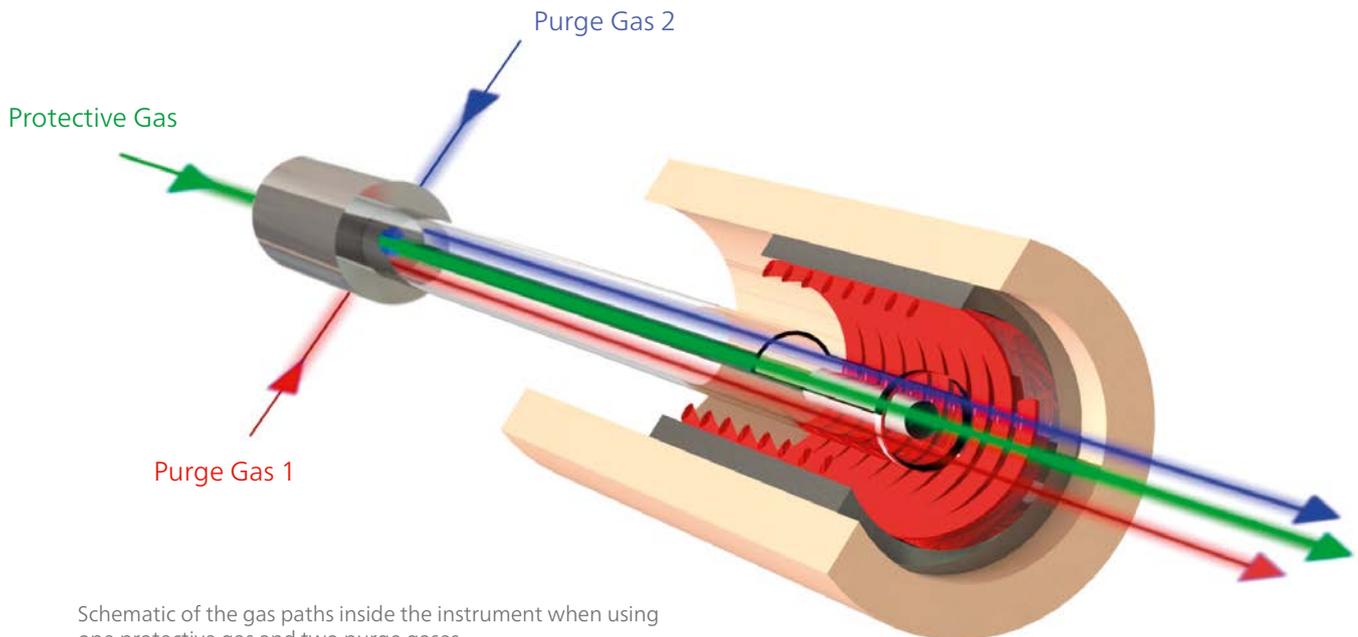

Schematic of the gas paths inside the instrument when using one protective gas and two purge gases

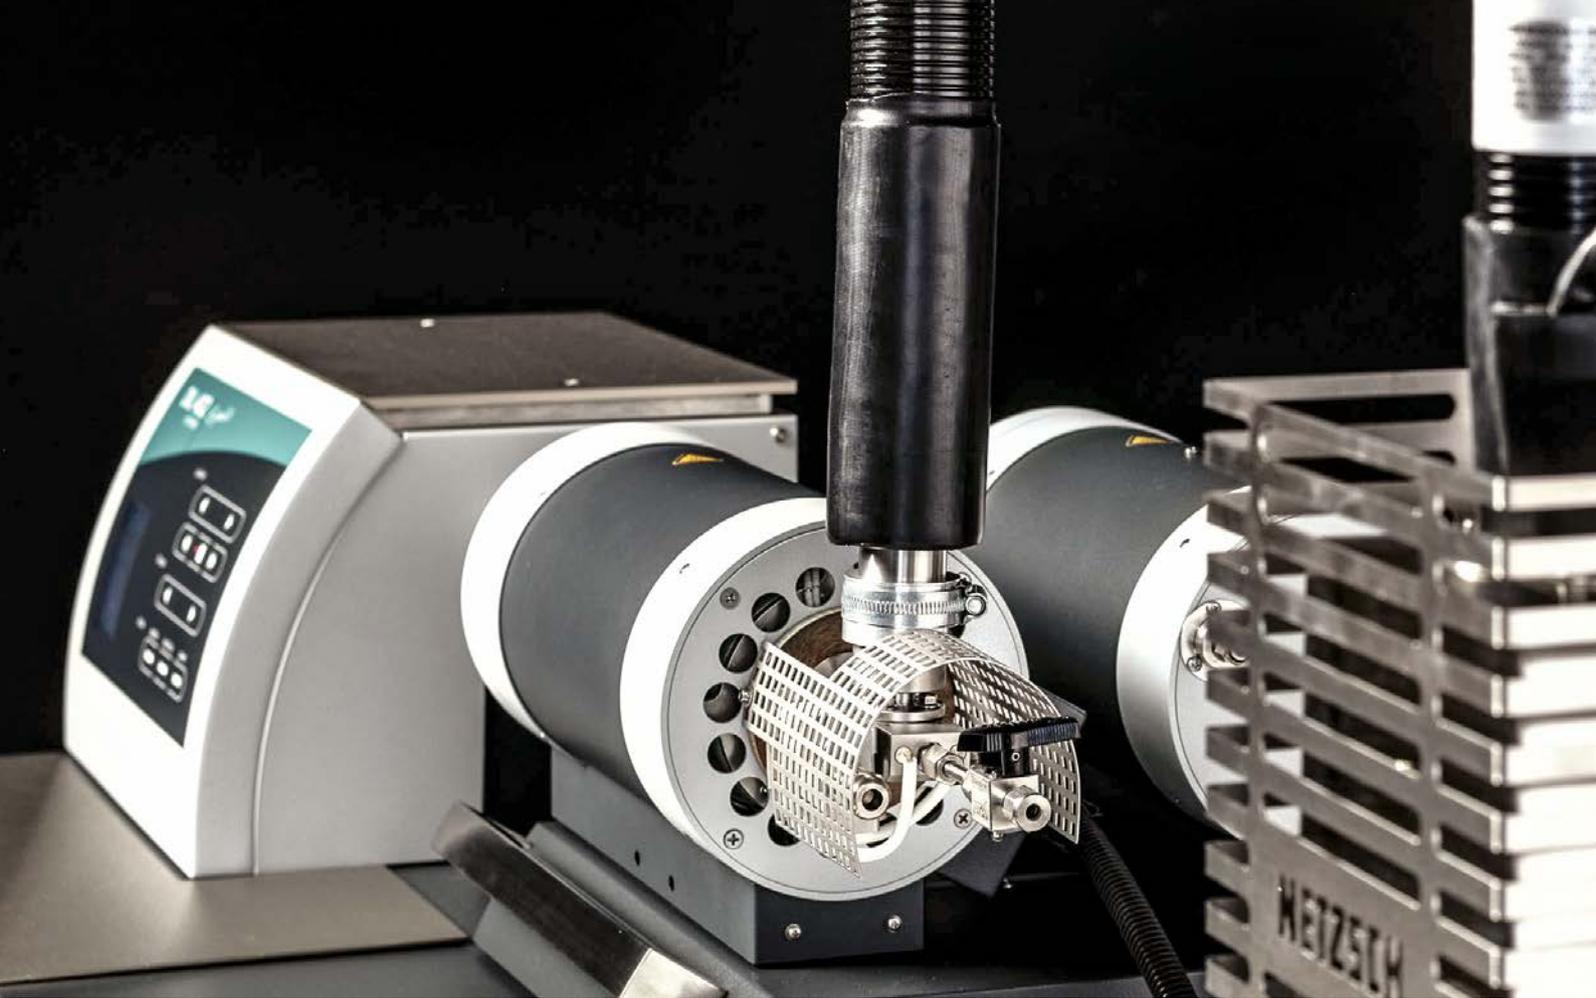

Silicon carbide furnace with transfer line connected for evolved gas analysis

### Vacuum-tight Design for Best Sample Conditions

The instrument can be equipped with evacuation systems such as *AutoVac* for fast evacuating and gas-refilling as well as measurements under vacuum.


### Oxygen-Free Measurement for Investigating Metals and Alloys

During the test run, in order to keep the residual oxygen concentration at the lowest possible level, the *OTS*<sup>®</sup> (Oxygen Trap System) can be applied. A getter ring on a ceramic substrate is mounted in the sample carrier tube and traps all oxygen residue within the inert purge gas.

### Identifying by Evolved Gas Analysis

The vacuum-tight design of the DIL 402 *Expedis*<sup>®</sup> is ideally suited for connection to a QMS or to an FT-IR via capillary coupling to the SiC furnace. Outgassing of impurities, additives, organic binders and/or decomposition products can thus be studied.

# DIL 402 *Expedis*<sup>®</sup> Supreme Glovebox Version

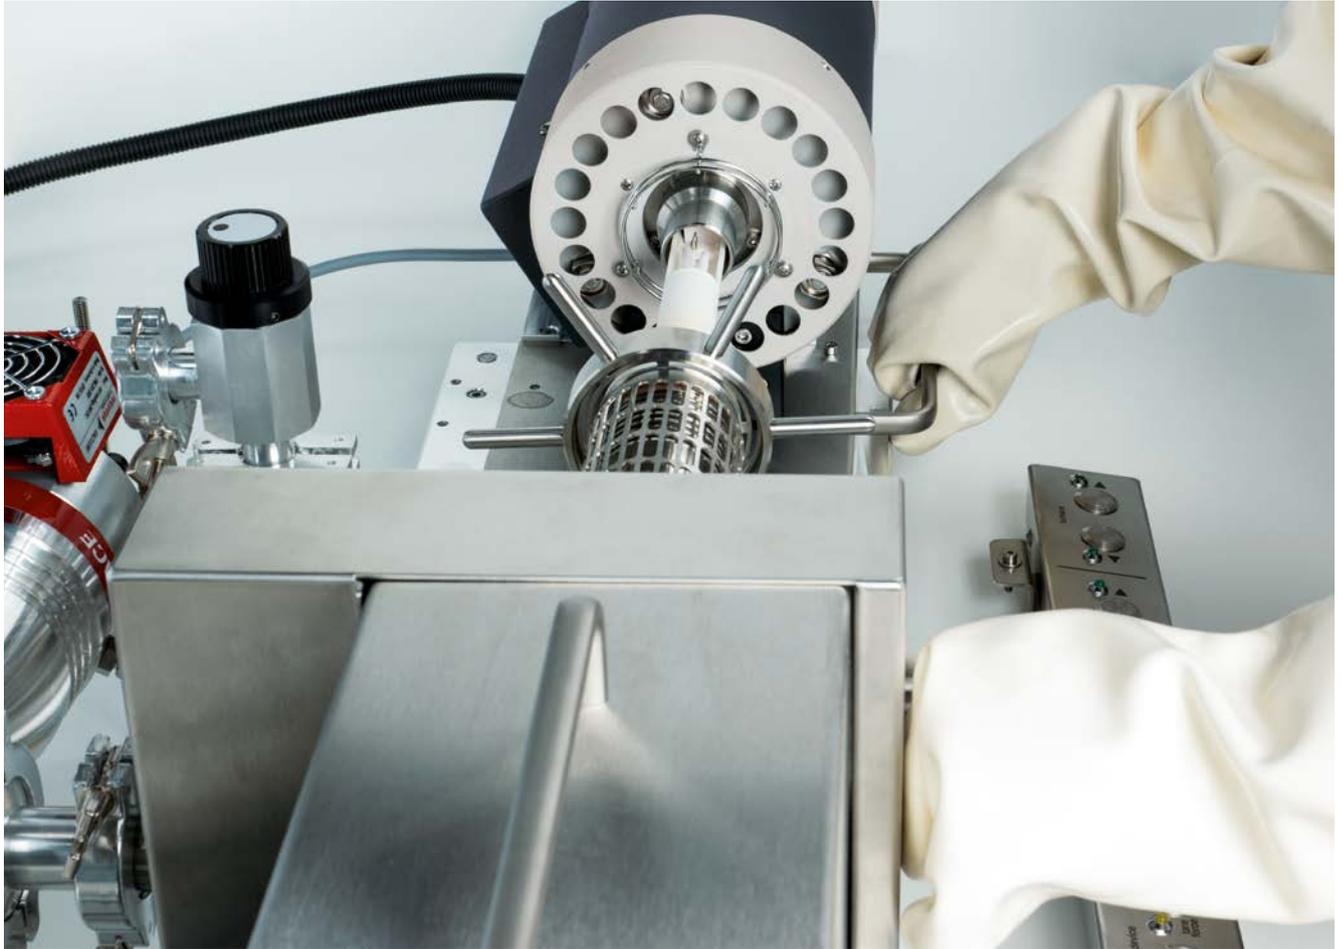

## For Investigations Requiring Special Care

In cases where materials are very sensitive to oxygen or humidity, or operators have to be protected from sample properties, the challenge can often only be managed by using a glovebox. The DIL 402 *Expedis*<sup>®</sup> Supreme Glovebox Version was specifically developed for such applications. It is a must for gloveboxes which cannot be opened anymore after implementation.

The entire casing of the dilatometer is made of stainless steel. There are therefore no plastic parts to potentially interact with samples or the environment.

For measurements up to 1650°C (furnace temperature) in an argon atmosphere, NETZSCH offers a rhodium furnace specially dedicated to this task.

## Comfortable Handling

Working in a glovebox often significantly restricts an operator's mobility, but the glovebox version of the DIL 402 *Expedis*<sup>®</sup> *Supreme* provides large, easily accessible buttons and allows for smooth operation.

The electronics of the system are separate from the mechanical parts wherever possible and designed for being positioned outside the glovebox.

For additional convenience, a remote control unit (optional) allows for controlling the movement of the pushrod or the movement of the furnace (optional) from outside the glovebox. This is especially advantageous if the dilatometer and the electronics are not together within the user's operational radius.

Alternatively, a separate control panel for working inside the glovebox, with large buttons and stainless steel casing, is available. It can be positioned by the user wherever it fits and handled with gloves. There is therefore no need to remove the gloves in order to move the pushrod or the furnace.

The *MultiTouch* function (see page 11) ensures that the sample is in an optimum position after insertion, eliminating any need to tap on the sample holder or the instrument.

The sample holders are available as single or dual systems. In order to make sample holder exchange as simple as possible, the furnace is rotatable and only toggle screws or knurled screws, which can be handled easily with gloves, are used.



DIL 402 *Expedis*<sup>®</sup> *Supreme* Glovebox Version with separate control panel (option) for use inside the glovebox



DIL 402 *Expedis*<sup>®</sup> *Supreme* Glovebox Version with remote control unit (option) for use outside the glovebox

# Sophisticated Solutions for Ambitious Tasks

# DIL 402 *Expedis*<sup>®</sup> *Supreme* HT up to 2800°C

## Broadest Application Range

Two graphite furnaces with end temperatures of 2400°C and 2800°C provide the appropriate configuration for measuring the thermal expansion of metals, alloys, ceramics and composites in applications such as aerospace, power generation, the oil and gas industry or demanding research. However, via an adapter, each of these graphite furnaces can be replaced with a standard furnace such as SiC, SiO<sub>2</sub>, Cu or steel.

The opposite is also feasible: A DIL 402 *Expedis*<sup>®</sup> *Supreme* HT measuring part with a standard furnace can be subsequently retrofitted with a high-temperature furnace.

## Pyrometer for Detection of the Highest Temperatures

Since W-Rh thermocouples can react with graphite above 2000°C, the sample temperature of the DIL 402 *Expedis*<sup>®</sup> *Supreme* HT is measured optically with a high-performance pyrometer from room temperature onward.

## Refined Safety System

An elaborate safety system monitors the cooling water and purge gas flow throughout the measurement.

## Variable Gas Atmosphere Is Key

In the DIL 402 *Expedis*<sup>®</sup> *Supreme* HT instrument, the sample chamber and furnace chamber are always separated by means of a protective tube (glassy carbon or alumina). This allows for the use of a different atmosphere around the sample than around the heating elements. In combination with an alumina protective tube (maximum furnace temperature: 1680°C), even an air atmosphere can be applied to the sample.


The optional *AutoVac* system for evacuating and refilling the sample chamber along with integrated purging of the pyrometer window effectively supports the direct switch between oxidizing and inert conditions.





DIL 402 *Expedis*<sup>®</sup> Supreme HT with 2800°C furnace. Due to the weight of this high-temperature furnace plus peripheral devices, the furnace sliding carrier is designed for one furnace only.

## For Horizontal Dilatometers Widest Temperature Range on the Market

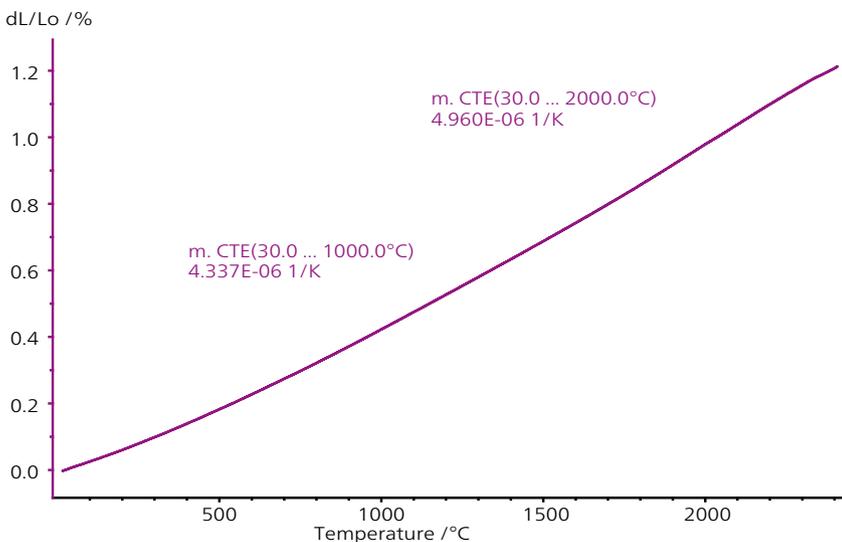

DIL measurement on recrystallized silicon carbide (RSiC), graphite sample holder, graphite protective plates (between the sample and sample holder/pushrod), original sample length: 18.98 mm, He atmosphere (50 ml/min), 10 K/min heating rate

### Recrystallized Silicon Carbide up to 2400°C

Recrystallized SiC (RSiC) sintered material is a technical ceramic often manufactured at temperatures around 2400°C. During sintering, a mixture of fine- and coarse-grained powder is transformed nearly shrinkage-free to a compact SiC matrix.

In the present case, the sample shows solely expansion over the entire temperature range from RT to 2400°C with CTE values of  $4.337 \times 10^{-6}$  1/K (between 30°C and 1000°C) and  $4.960 \times 10^{-6}$  1/K (between 30°C and 2000°C).

# Proteus<sup>®</sup> Software

## Best Practice for Measurement and Evaluation

The unique *Proteus*<sup>®</sup> 7 dilatometer software offers everything a user could ever want and need: It runs smoothly, provides reliable results, and it is fast and efficient. It provides a large range of functions, but – at the same time – offers a clearly-arranged user interface. Additionally, it is intuitive and thus easy to learn.

But ... that's not all. There are some more options inside which impress even the most experienced operators – particularly the *Density Determination*, the patented *c-DTA*<sup>®</sup> and the innovative *Identify* software features. (More about *Identify* on pages 20/21).


### Density Determination

This program add-on allows determination of the density change of samples with varying consistency, i.e., solids, viscous materials such as pastes, liquids or melts as well as the volumetric expansion of isotropic materials.

### Patented\* *c-DTA*<sup>®</sup>

The *c-DTA*<sup>®</sup> signal gives the opportunity for simultaneous analysis of length changes and endothermal/exothermal effects. It can also be used for temperature calibration.

\* DE102013100686

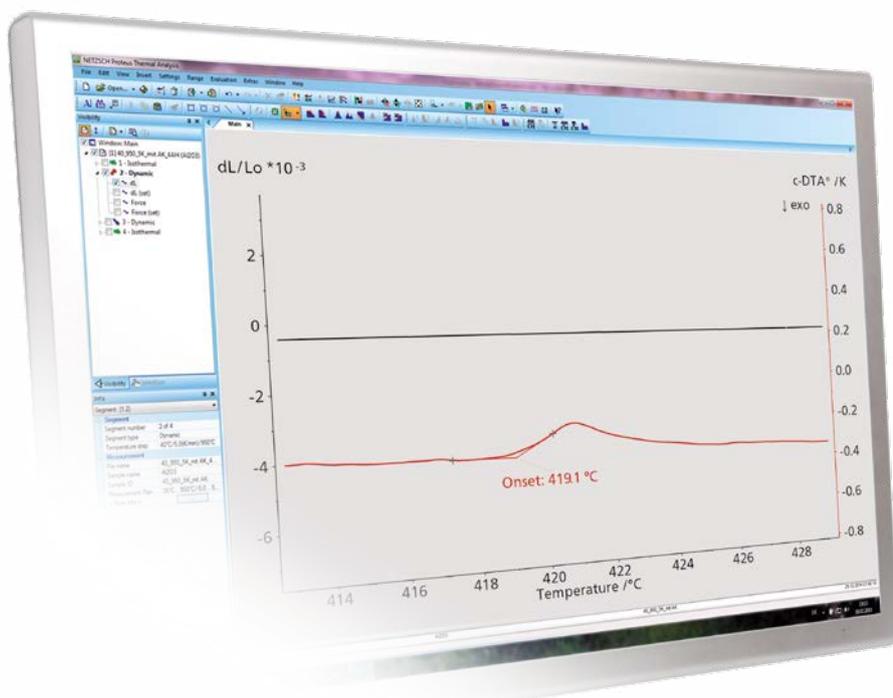

### Special Features of the *Proteus*® Software for DIL 402 *Expedis*® *Select* and *Supreme* at a Glance\*

Software-controlled force adjustment  
(incl. constant forces, ramps, steps)

Force modulation

*Density Determination*

c-DTA® for temperature calibration or determination of  
caloric effects

RCS Rate-Controlled Sintering

*Identify* identification of unknown  $\Delta L/L_0$  curves through  
database comparison

### Advanced Software (for extended evaluation of the measuring data)\*

Kinetics Neo

*PeakSeparation* (for processing the 1<sup>st</sup> derivative)

\* for information which software features are included as standard  
and which ones are optionally available, please see page 25

INFORMATION AT A GLANCE  
GRAPHICAL PRESENTATIONS  
SOPHISTICATED SOFTWARE  
MULTIPLE WINDOWS  
METHOD-BASED MEASUREMENTS  
COMPREHENSIVE TEMPERATURE PROGRAMS  
LOOP PROGRAMMING  
(MEASUREMENT) STATUS WINDOW  
COMPARATIVE ANALYSIS  
SIMULTANEOUS ANALYSIS  
TIME AND TEMPERATURE SCALING  
EXTRAPOLATION OF COEFFICIENTS  
CHANGE OF UNITS  
ZOOM FUNCTION  
SOFTENING POINT DETECTION  
**RATE-CONTROLLED SINTERING**  
DATA EXPORT  
TABULAR PRINTOUT OF RESULTS  
**IDENTIFY**  
OPTIMIZED DATA STORAGE  
**DENSITY DETERMINATION**  
EVALUATION OF ARRAY OF  
UNLIMITED CURVES  
XY-OFFSET SHIFT  
**c-DTA**®  
SET COMMENTS  
GET OFFSET FROM RAW DATA  
EXTRAPOLATION OF ONSET  
DIN AND ASTM CORRECTIONS  
GAS MANAGER  
CONTROLLABLE GAS BY SEGMENT  
AUTOMATIC SAMPLE LENGTH DETECTION  
INPUT ASSISTANT  
SNAPSHOT  
JUMP FUNCTIONS  
STATUS MESSAGES BY EMAIL  
SIMULTANEOUS LOADING OF MULTIPLE FILES  
PIP AND FLIP  
AUTO-ARRANGING OF CURVES  
IMPORT OF STANDARD TABLES  
EVALUATION ACROSS ALL SEGMENTS  
IMPORT AND EXPORT ROUTINES  
ADJUSTABLE SMOOTHING FILTERS  
SPLINE INTERPOLATION

# Identify

## Built-In Thermal Analysis Expertise

The unparalleled *Identify*, for the identification and interpretation of DIL measurements includes several NETZSCH libraries with hundreds of entries from the ceramic, inorganic, metal, alloy, and polymer or organic fields. Additionally, user-specific libraries can be created. They can be shared with other users within a computer network.

*Identify* allows the identification of unknown samples from the absolute values, the slope or the shape of a measured curve. This will also open up the opportunity to compare known samples against a variety of other samples, enabling one to make a statement about material quality. Finally, all measurements can be stored in the extensive database and are always available for identification or quality comparison.



*Identify* provides all information with one single click



## Identification

of unknown measurement curves

## Quality Control

via agreement between the current measurement  
and selected database entries



## Archiving functionality

for present measurements and existing  
database entries



# Applications

## Thermal Behavior of Carbon Fiber-Reinforced Carbon up to 2000°C

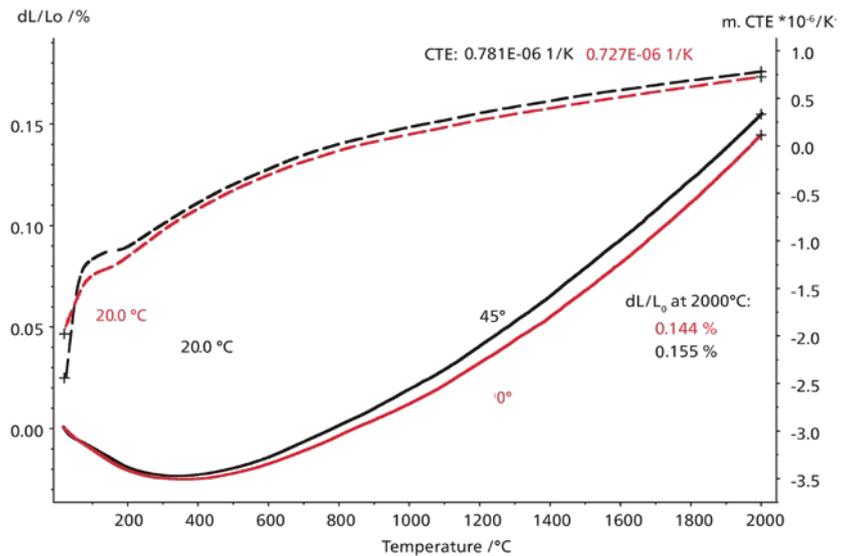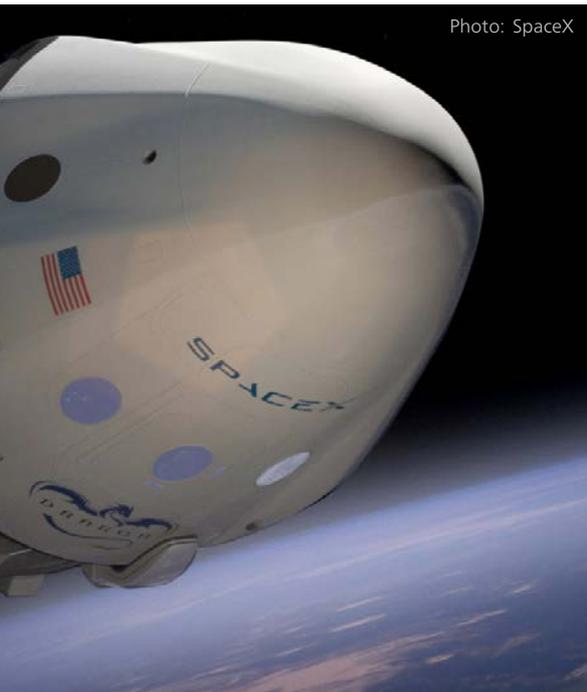

Comparison of two expansion measurements of a C/C material, measured 45° (black) and 0° (red) relative to the fiber direction; heating rate: 5 K/min, He atmosphere, constant contact force: 225 mN, graphite sample holder. Displayed are the relative length changes (solid lines) and the mean coefficients of thermal expansion (m. CTE) based on 20°C (dashed lines).

This composite material is composed of a matrix of pure carbon to which carbon fibers are added. It exhibits high mechanical strength associated with high temperature stability.

The thermal expansion of C/C materials depend on their fiber architecture. In the present case, experiments with angles of 45° (black) and 0° (red) relative to the fiber orientation were conducted. Both curves depict a characteristic behavior of such fiber-reinforced composites: passing a length change minimum between approx. 300°C and 400°C followed by expansion.

At 2000°C, the relative length change ( $dL/L_0$  in %) as well as the corresponding mean CTE of the specimen cut out with a 45° angle relative to the fiber direction (black) are just about 7% higher (0.155% and  $0.781 \times 10^{-6} \text{ 1/K}$ ) than that of the sample cut out with a 0° angle (red, 0.144% and  $0.727 \times 10^{-6} \text{ 1/K}$ ). This suggests a quite low dependency of the material properties within these spatial directions.





## Volumetric Expansion of an Aluminum Alloy into the Melt


The behavior of an aluminum-based alloy during heating is illustrated here. Displayed are the volumetric expansion ( $dV/V_0$ , black) and the density change (red) which can both be calculated from the measured thermal expansion data by using the NETZSCH *Density Determination* software.

After an initial linear expansion, the aluminum alloy starts to melt at 559°C (extrapolated onset temperature of the *c-DTA*® signal in dashed blue). For realizing such an experiment, a special container (here alumina, see photo) is necessary.

During melting, a strong expansion occurs representing the mushy region in which liquid and solid state are present together. Above 622°C, the entire sample is molten.

While the volume increases, the initial density drops down for about 10% (from 2.66 g/cm<sup>3</sup> to 2.40 g/cm<sup>3</sup>) until the end of the measurement.

The *c-DTA*® curve (blue) clearly shows the melting range by endothermic effects.

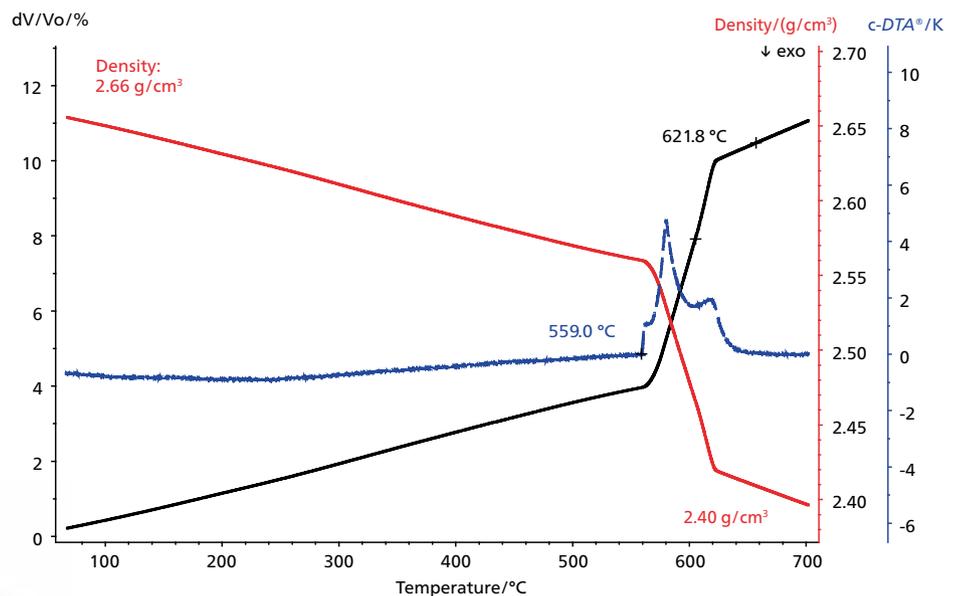

Thermal behavior of an aluminum-based alloy, heating rate: 5 K/min, He atmosphere, constant contact force: 250 mN, alumina sample holder, alumina container. Displayed are the volumetric expansion (black solid line), the curve of the calculated density change (red solid line) as well as the *c-DTA*® curve (blue dashed line).



# Applications

## Without Oxidation to the Highest Temperatures!


Tungsten is a metal very sensitive to oxidation. But due to the vacuum-tight design of the *Expedis® Supreme*, the material can be measured in pure He atmosphere (in combination with *OTS®* – Oxygen Trap System) to get its true expansion behavior. There is no need of reducing atmosphere to suppress superficial oxidation (which would change the color of the sample).

### Comparison of Measurement and Literature


Measured CTE  
between 20°C and 1500°C  
 **$5.143 \times 10^{-6} \text{ 1/K}$**

Literature values  
(NIST standard table)  
 **$5.129 \times 10^{-6} \text{ 1/K}$**

Difference between  
measurement and literature  
 **$1.4 \times 10^{-8} \text{ 1/K}$**

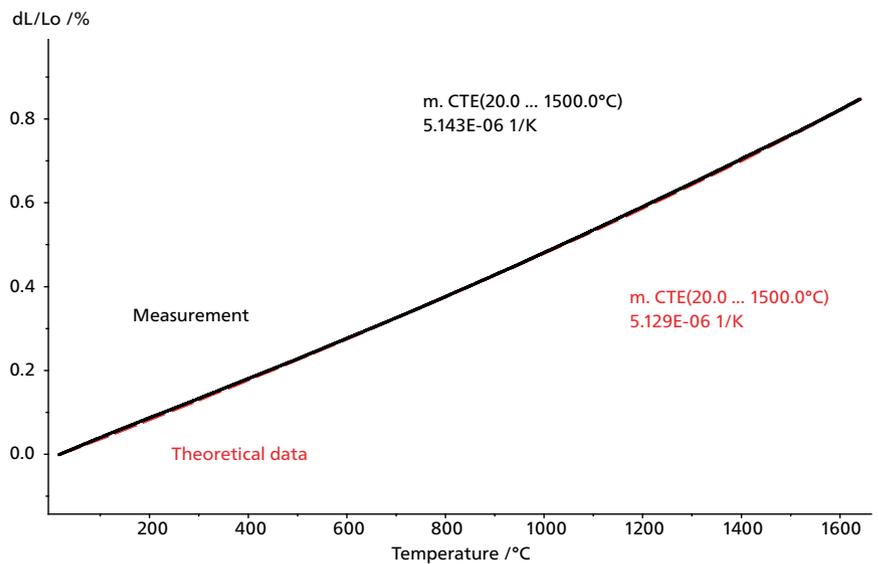

Thermal behavior of tungsten, sample length: 25.00 mm, heating rate: 5 K/min, He atmosphere, constant contact force: 250 mN, alumina sample holder. Displayed are the length change of the sample (black solid line) together with the tabulated theoretical data (red dashed line, NIST standard table).

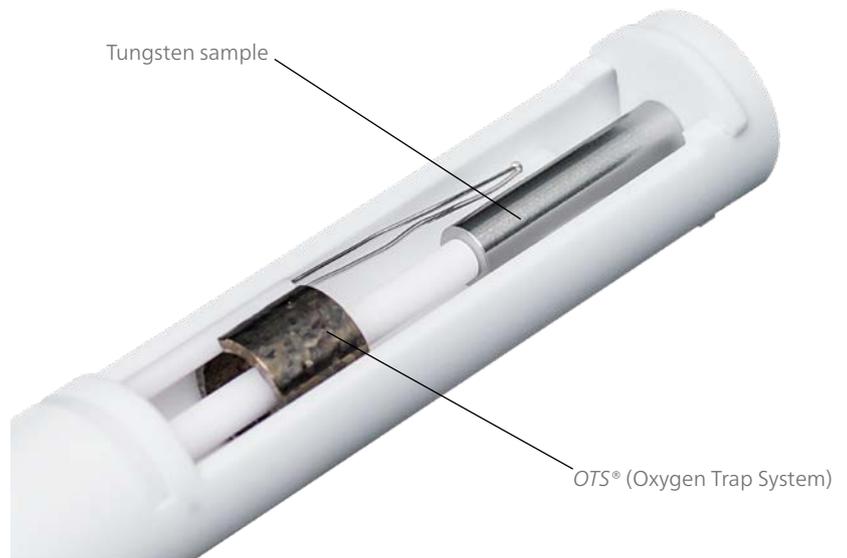

The picture on the left side illustrates two tungsten samples after the experiment. The used tungsten samples were measured up to 1640° C. The right sample is corroded because of non-oxygen free atmosphere during measurement. The left sample, also shown in the picture above, is still shiny due to a measurement in oxygen-free atmosphere.

# Configurations

Feature	Supreme	Select	Supreme HT
Max. temperature range	-180°C ... 2000°C	-180°C ... 1600°C	(-180°C)* ... RT ... 2800°C
Measuring range	50 mm (± 25 000 µm)	20 mm (± 10 000 µm)	50 mm (± 25 000 µm)
ΔL Resolution (over entire measuring range)	0.1 nm	1 nm	0.1 nm
Double furnace sliding carrier	■	■	N/A
Motorized furnace operation	□	□	■
Vacuum-tight design	■	■	■
Automatic Evacuation System – <i>AutoVac</i>	□	□	□
Mass Flow Controller (MFC) – single/triple	■ / □	■ / □	■ / □
Available Cooling Devices	Vortex, LN <sub>2</sub>	Vortex, LN <sub>2</sub>	Vortex, LN <sub>2</sub>
Electrical temperature control of the measuring cell	■	■	■
Force change (ramp, step at each new segment)	■	■	■
Force modulation	■	□	■
Single/double DIL	■ / □	■ / □	■ / □
Automatic sample length detection	■	■	■
Softening Point detection	■	■	■
<i>Density Determination</i>	■	□	■
<i>c-DTA</i> <sup>®</sup>	■	□	■ **
RCS (Rate-Controlled Sintering)	■	□	■
<i>Identify</i>	■	□	■
Evolved gas analysis (coupling with GC-MS/QMS and/or FT-IR) – for SiC furnace	□	□	□

\* DIL 402 *Expedis*<sup>®</sup> Supreme HT with adapter for standard furnaces

\*\* Not above 2000°C, only by thermocouple operation

Both instrument models work on the basis of DIN 51045, ASTM E228, ASTM D696 or DIN EN 821.

- Included in standard configuration
- Optional
- N/A Not applicable

# Technical Specifications

## DIL 402 Expedis® Supreme, Supreme HT and Select

Design	Pushrod dilatometer, single or dual system
Furnaces	Different types, interchangeable (for <i>Supreme</i> HT partially with adapter): steel, copper, SiO <sub>2</sub> , SiC (optional furnace for fast cooling available), Rh; graphite (only for <i>Supreme</i> version)
Heating rates	Depending on furnace type: <ul style="list-style-type: none"> <li>Steel, copper, fused silica, silicon carbide: 0.001 ... 50 K/min</li> <li>Graphite: 0.001 ... 100 K/min</li> </ul>
Cooling systems	Depending on furnace: Vortex, LN <sub>2</sub> -device, air compressor SiO <sub>2</sub> , Al <sub>2</sub> O <sub>3</sub> , graphite ( <i>Supreme</i> version), user interchangeable
Sample holder systems	All sample holders are available as <ul style="list-style-type: none"> <li>Single system (one pushrod)</li> <li>System with two pushrods usable in dual or differential mode</li> <li>Al<sub>2</sub>O<sub>3</sub> tension sample holder*</li> </ul> SiO <sub>2</sub> and Al <sub>2</sub> O <sub>3</sub> sample holders can be purchased as tube or rod design
Sample dimensions	Max. length: 52 mm (graphite furnace: 25 mm) Diameter (single): standard 12 mm, optional 19 mm Diameter (dual): 8 mm
Automatic sample length determination	Yes, in expansion mode
Displacement system	<i>NanoEye</i>
Temperature accuracy / precision / resolution	1 K / 0.1 K / 0.001 K
Thermal stability (isothermal)	± 0.02 K
Temperature calibration	Displacement method (by using metal references and protective disks) or via <i>c-DTA</i> ® (optional for <i>Select</i> version; incl. endo/exothermal effects)
Measuring range	± 25000 µm ( <i>Supreme</i> version) ± 10000 µm ( <i>Select</i> version)
ΔL Resolution	0.1 nm ( <i>Supreme</i> version) 1 nm ( <i>Select</i> version)
ΔL/L <sub>0</sub> Repeatability	0.001 %, absolute value
ΔL/L <sub>0</sub> Accuracy	0.002 %, absolute value
Force range (load at the sample)	10 mN ... 3 N (valid for compressive and tensile force depending on the sample holder)
Change of force	<i>Supreme</i> version: various options, incl. modulated forces <i>Select</i> version: changeable per segment (constant & ramp)
Force resolution	0.001 mN
Gas atmosphere	Inert, oxidizing, reducing, vacuum
Gas control	MFC <ul style="list-style-type: none"> <li>Standard: 1 x protective gas</li> <li>Optional: 1 x protective gas, 2 x purge gas</li> </ul>
Oxygen Trap System (OTS®)	Optional, for single and for dual sample holder systems
Software	Windows 7 32/64 bit Professional®, Enterprise® and Ultimate®, Windows 8.1 Pro® and Enterprise®, Windows 10 Pro® and Enterprise®

\* Please note, using the tension sample holder has an influence on the noise behavior as well as the temperature range when using the copper furnace.



All over the world, the name NETZSCH stands for comprehensive support and expert, reliable service, both before and after sale. Our qualified personnel from the technical service and application departments are always available for consultation. In special training programs tailored for you and your employees, you will learn to tap the full potential of your instrument.

To maintain and protect your investment, you will be accompanied by our experienced service team over the entire life span of your instrument.

# Expertise in SERVICE

## TECHNICAL SERVICE



Maintenance and Repair



Software Updates



Exchange Service



IQ/OQ Documents



Calibration Service



Spare Part Assistance



Moving Service

## TRAINING



Training



Comprehensive Instrument and Method Training

## LABORATORY



Application Service and Contract Testing



The NETZSCH Group is an owner-managed, international technology company with headquarters in Germany. The Business Units Analyzing & Testing, Grinding & Dispersing and Pumps & Systems represent customized solutions at the highest level. More than 3,700 employees in 36 countries and a worldwide sales and service network ensure customer proximity and competent service.

Our performance standards are high. We promise our customers Proven Excellence – exceptional performance in everything we do, proven time and again since 1873.

When it comes to Thermal Analysis, Calorimetry (adiabatic & reaction), the determination of Thermophysical Properties, Rheology and Fire Testing, NETZSCH has it covered. Our 50 years of applications experience, broad state-of-the-art product line and comprehensive service offerings ensure that our solutions will not only meet your every requirement but also exceed your every expectation.

## Proven Excellence.■

NETZSCH-Gerätebau GmbH  
Wittelsbacherstraße 42  
95100 Selb  
Germany  
Tel.: +49 9287 881-0  
Fax: +49 9287 881 505  
at@netsch.com

**NETZSCH®**

[www.netsch.com](http://www.netsch.com)